




Enabling Legendary Discovery™

## **LEGEND MAX™**

ELISA Kit with Pre-coated Plates



### **Mouse CCL11 (Eotaxin)**

Cat. No. 443907      1 Plate

443908      5 Plates

ELISA Kit for Accurate Quantitation of Mouse  
CCL11 from Cell Culture Supernatant, Serum, Plasma,  
and Other Biological Fluids

BioLegend, Inc.  
[biolegend.com](http://biolegend.com)

***It is highly recommended that this manual be read in its entirety before using this product. Do not use this kit beyond the expiration date.***

*For Research Purposes Only. Not for use in diagnostic or therapeutic procedures. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of BioLegend is strictly prohibited.*



<b>Table of Contents</b>	<b>Page</b>
Introduction.....	2
Materials Provided.....	2
Materials to be Provided by the End-User.....	3
Storage Information.....	3
Health Hazard Warnings.....	3
Specimen Collection and Handling.....	4
Reagent and Sample Preparation.....	4
Assay Procedure.....	5
Assay Procedure Summary.....	7
Calculation of Results.....	8
Typical Data.....	8
Performance Characteristics.....	9
Specificity.....	9
Sensitivity.....	9
Linearity.....	9
Recovery.....	9
Intra-Assay Precision.....	9
Inter-Assay Precision.....	9
Biological Samples.....	10
Troubleshooting Guide.....	11
ELISA Plate Template.....	13

# LEGEND MAX™ Mouse CCL11 ELISA Kit

## Introduction:

CCL11, also known as Eotaxin, is a small cytokine belonging to the CC chemokine family. The full length of CCL11 is 97 amino acids (aa) with a 23 aa signal peptide, which is cleaved to generate a 74 aa mature protein. The molecular mass of CCL11 is about 10 kD, and its gene is located on the q arm of chromosome 17. CCL11 expression has been found in normal tissues such as smooth muscle and small intestine. Endothelial cells, smooth muscle cells, epithelial cells, alveolar macrophages and eosinophils are known to produce CCL11. Mouse CCL11 shares 61% and 96% amino acid sequence identity to both human and rat, respectively.

CCL11 is produced when inflammatory cytokines, such as IL-5 and TNF- $\alpha$ , stimulate lung endothelial cells, fibroblasts, and smooth muscle cells in response to allergens. As a potent eosinophil chemoattractant, via binding to its major receptor, CCR3, CCL11 efficiently induces the accumulation of eosinophils, a response associated with allergic inflammation. Therefore, atopic dermatitis, asthma, and parasitic infections are a few of the eosinophilic inflammatory diseases directly related to CCL11. In addition, CCL11 induces the formation of blood vessels and other angiogenic responses that are accompanied by inflammatory infiltration, and is also involved in regulation of tumor development.

The LEGEND MAX™ Mouse CCL11 ELISA kit is a Sandwich Enzyme-Linked Immunosorbent Assay (ELISA) with a 96-well strip plate that is pre-coated with a rat monoclonal anti-mouse CCL11 antibody. The Detection Antibody is a biotinylated goat polyclonal anti-mouse CCL11 antibody. This kit is specifically designed for the accurate quantitation of mouse CCL11 from cell culture supernatant, serum, plasma, and other biological fluids. This kit is analytically validated with ready-to-use reagents.

## Materials Provided:

Description	Quantity (1 plate)	Quantity (5 plates)	Volume (per bottle)	Part #
Anti-Mouse CCL11 Pre-coated 96 well Strip Microplate	1 plate	5 plates		76522
Mouse CCL11 Detection Antibody	1 bottle	5 bottles	12 mL	76523
Mouse CCL11 Standard	1 vial	5 vials	lyophilized	76525
Avidin-HRP	1 bottle	5 bottles	12 mL	77897
Assay Buffer B	1 bottles	5 bottles	25 mL	79128
Wash Buffer (20X)	1 bottle	5 bottles	50 mL	78233
Substrate Solution F	1 bottle	5 bottles	12 mL	79132
Stop Solution	1 bottle	5 bottles	12 mL	79133
Plate Sealers	1 pack	5 packs		78101

## LEGEND MAX™ Mouse CCL11 ELISA Kit

### Materials to be Provided by the End-User:

- Microplate reader able to measure absorbance at 450 nm
- Adjustable pipettes to measure volumes ranging from 1 µL to 1,000 µL
- Deionized water
- Wash bottle or automated microplate washer
- Log-Log graph paper or software for data analysis
- Tubes to prepare standard dilutions
- Timer
- Plate Shaker
- Polypropylene vials

### Storage Information:

Store unopened kit components between 2°C and 8°C. Do not use this kit beyond its expiration date.

Opened or Reconstituted Components	
Microplate wells	If not all microplate strips are used, remove the excess strips by pressing up from underneath each strip. Place excess strips back in the foil pouch with the included desiccant pack and reseal. Store between 2°C and 8°C for up to one month.
Standard	The remaining reconstituted standard stock solution can be aliquoted into polypropylene vials and stored at -70°C for up to one month. Avoid repeated freeze-thaw cycles.
Detection Antibody	Store opened reagents between 2°C and 8°C and use within one month.
Avidin-HRP	
Assay Buffer B	
Wash Buffer (20X)	
Substrate Solution F	
Stop Solution	

### Health Hazard Warnings:

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin. Refer to the MSDS online at BioLegend's website for details ([www.biolegend.com/msds](http://www.biolegend.com/msds)).
2. Substrate Solution F is harmful if inhaled or ingested. Avoid skin, eye and clothing contact.
3. To reduce the likelihood of blood-borne transmission of infectious agents, handle all serum, plasma and other biological fluids in accordance with

## LEGEND MAX™ Mouse CCL11 ELISA Kit

NCCLS regulations.

4. Stop Solution contains strong acid and is corrosive. *Wear eye, hand, and face protection when handling, and follow state and county regulation for disposal.*
5. Before disposing of the plate, rinse it with an excess amount of tap water.

### **Specimen Collection and Handling:**

Specimens should be clear and non-hemolyzed. If possible, unknown samples should be run at a number of dilutions to determine the optimal dilution factor that will ensure accurate quantitation.

Cell Culture Supernatant: If necessary, centrifuge all samples to remove debris prior to analysis. *It is recommended that samples be stored at < -70°C. Avoid repeated freeze-thaw cycles.*

Serum: Use a serum separator tube and allow clotting for at least 30 minutes, then centrifuge for 10 minutes at 1,000 x g. Remove serum layer. *Assay immediately or store serum samples at < -70°C. Avoid repeated freeze-thaw cycles.*

Plasma: Collect blood samples in heparin, citrate or EDTA-containing tubes. Centrifuge for 10 minutes at 1,000 x g within 30 minutes of collection. *Assay immediately or store plasma samples at < -70°C. Avoid repeated freeze-thaw cycles.*

### **Reagent and Sample Preparation:**

Note: All reagents should be diluted immediately prior to use.

1. Dilute the 20X Wash Buffer to 1X with deionized water. For example, make 1 liter of 1X Wash Buffer by adding 50 mL of 20X Wash Buffer to 950 mL of deionized water. If crystals have formed in the 20X Wash Buffer, bring to room temperature and mix until dissolved.
2. Reconstitute the lyophilized Mouse CCL11 Standard by adding the volume of Assay Buffer B to make the 20 ng/mL standard stock solution (Refer to LEGEND MAX Kit Lot-Specific Certificate of Analysis/LEGEND MAX Kit Protocol). Allow the reconstituted standard to sit at room temperature for 15 minutes, then briefly vortex to mix completely.
3. For cell culture supernatant samples, the end user may need to determine the dilution factor needed in a preliminary experiment. If dilutions are necessary, samples should be diluted in the corresponding cell culture medium.
4. CCL11 levels in serum and plasma samples vary. It is recommended to run several dilutions to determine the optimal dilution factor for each sample. A 5-fold dilution is suggested for serum or plasma. All dilutions should be


## LEGEND MAX™ Mouse CCL11 ELISA Kit

prepared in Assay Buffer B. For example, 50  $\mu\text{L}$  of serum sample should be added to 200  $\mu\text{L}$  of Assay Buffer B to make a 1:5 dilution.

### Assay Procedure:

Note: Do not mix reagents from different kits or lots. Reagents and/or antibodies from different manufacturers should not be used with this kit.

1. Bring all reagents to room temperature prior to use. It is strongly recommended that all standards and samples be run in duplicate. A standard curve is required for each assay.
2. If not all microplate strips will be used, remove the excess strips by pressing up from underneath each strip. Place excess strips back in the foil pouch with the included desiccant pack and reseal.
3. Prepare 1,000  $\mu\text{L}$  of the 400 pg/mL top standard by diluting 20  $\mu\text{L}$  of the standard stock solution in 980  $\mu\text{L}$  of Assay Buffer B. Perform six two-fold serial dilutions of the 400 pg/mL top standard in separate tubes using Assay Buffer B as the diluent. Thus, the mouse CCL11 standard concentrations in the tubes are 400 pg/mL, 200 pg/mL, 100 pg/mL, 50 pg/mL, 25 pg/mL, 12.5 pg/mL and 6.25 pg/mL, respectively. Assay Buffer B serves as the zero standard (0 pg/mL).

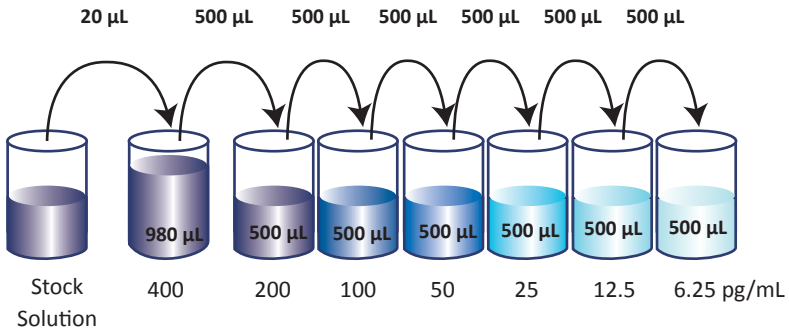

4. Add 50  $\mu\text{L}$  of Assay Buffer B to each well that will contain either standards or samples.
5. Add 50  $\mu\text{L}$  of standard dilutions or properly diluted samples to the appropriate wells.
6. Seal the plate with a Plate Sealer included in the kit and incubate the plate at room temperature for 2 hours while shaking at 200 rpm.
7. Discard the contents of the plate into a sink, then wash the plate 4 times with 1X Wash Buffer. Wash the plate with at least 300  $\mu\text{L}$  of 1X Wash Buffer per well and blot any residual buffer by firmly tapping plate upside down on absorbent paper. All subsequent washes should be performed similarly.


## LEGEND MAX™ Mouse CCL11 ELISA Kit

8. Add 100  $\mu$ L of Mouse CCL11 Detection Antibody solution to each well, seal the plate and incubate at room temperature for 1 hour while shaking.
9. Discard the contents of the plate into a sink, then wash the plate 4 times with 1X Wash Buffer as in step 7.
10. Add 100  $\mu$ L of Avidin-HRP solution to each well, seal the plate and incubate at room temperature for 30 minutes while shaking.
11. Discard the contents of the plate into a sink, then wash the plate 5 times with 1X Wash Buffer as in step 7. For this final wash, soak wells in 1X Wash Buffer for 30 seconds to 1 minute for each wash. This will help minimize background.
12. Add 100  $\mu$ L of Substrate Solution F to each well and incubate for 15 minutes in the dark. Wells containing mouse CCL11 should turn blue in color with intensity proportional to concentration. It is not necessary to seal the plate during this step.
13. Stop the reaction by adding 100  $\mu$ L of Stop Solution to each well. The well color should change from blue to yellow.
14. Read absorbance at 450 nm within 20 minutes. If the reader is capable of reading at 570 nm, the absorbance at 570 nm can be subtracted from the absorbance at 450 nm.




## Assay Procedure Summary


1. Add 50  $\mu$ L Assay Buffer B

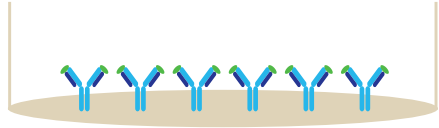


2. Add 50  $\mu$ L prepared standards or samples.  
Incubate 2 hrs, RT, shaking

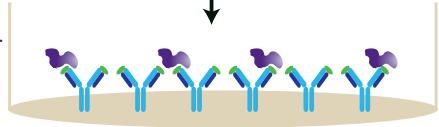


3. Wash 4 times  
Add 100  $\mu$ L Detection Antibody solution  
Incubate 1hr, RT, shaking

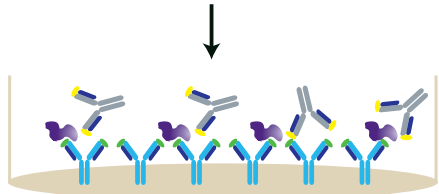


4. Wash 4 times  
Add 100  $\mu$ L Avidin-HRP solution  
Incubate 30 mins, RT, shaking

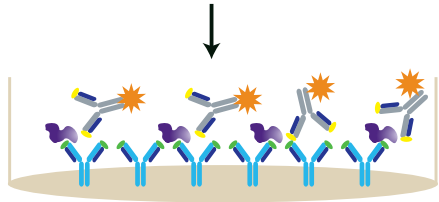

5. Wash 5 times  
Add 100  $\mu$ L Substrate Solution F  
Incubate 15 mins, RT, in the dark

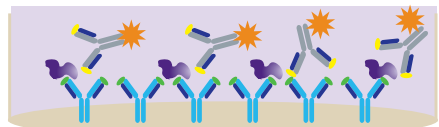

6. Add 100  $\mu$ L Stop Solution

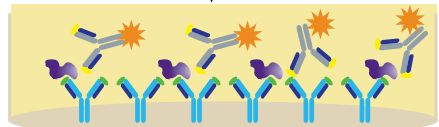

7. Read absorbance at 450 nm and 570 nm

# LEGEND MAX™ Mouse CCL11 ELISA Kit


## Calculation of Results:

The data can be best calculated with computer-based curve-fitting software using a 5- or 4-parameter logistics curve-fitting algorithm. If appropriate software is not available, use log-log graph paper to determine sample concentrations. Determine the mean absorbance for each set of duplicate or triplicate standards, controls, and samples. Plot the standard curve on log-log graph paper with antigen concentration on the X-axis and absorbance on the Y-axis. Draw a best fit line through the standard points. To determine the unknown antigen concentrations, find the mean absorbance value of the unknown concentration on the Y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the sample concentration.

If samples were diluted, multiply the concentration by the appropriate dilution factor. If a test sample's absorbance value falls outside the linear portion of the standard curve, the test sample needs to be re-analyzed at a higher (or lower) dilution as appropriate.

## Typical Data:

This standard curve was generated at BioLegend for demonstration purposes only. A standard curve must be run with each assay.

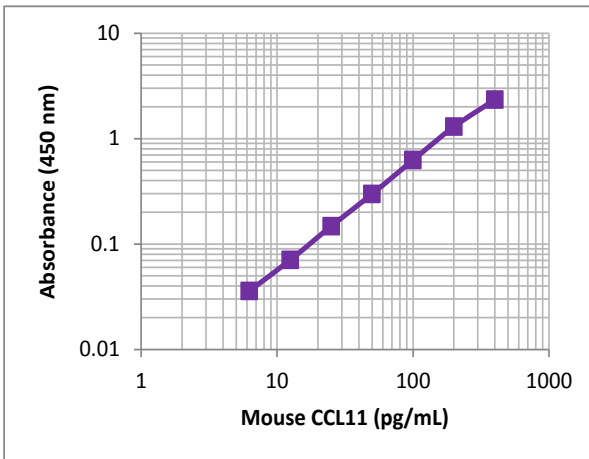

**Performance Characteristics:**

**Specificity:** No cross-reactivity was observed when this kit was used to analyze the following recombinant proteins, each at 50 ng/mL.

Human	CCL2, CCL5, CCL8
Rat	MIF, EPO, CXCL1, CCL20, GM-CSF, IGF-1, IL-2, TNF- $\alpha$ , TPO, KC, IL-13, IL-10, IL-18, IL-33, CCL20, MCP-1
Mouse	CCL1, CCL2, CCL7, CCL8, CCL9, CCL12, CCL17, CCL19, CCL20, CCL21, CCL22, CCL24, CCL25, CCL28, CXCL1, CXCL2, CXCL3, CXCL4, CXCL5, IFN- $\gamma$ , TNF- $\alpha$ , GM-CSF, EGF

This kit fully detects rat CCL11 protein and highly cross-reacts (27%) to human CCL11 protein. There was 0.05% and 0.1% cross reactivity to recombinant human CCL7 and CCL13, respectively.

**Sensitivity:** The average minimum detectable concentration of mouse CCL11 is  $0.825 \pm 0.386$  pg/mL.

**Linearity:** Pre-diluted mouse serum, plasma, and cell culture media were further diluted two, four, and eight fold with Assay Buffer B to produce sample concentrations within the dynamic range of the assay.

**Recovery:** Three levels of recombinant Mouse CCL11 (200 pg/mL, 50 pg/mL and 12.5 pg/mL) were spiked into pre-diluted mouse serum, plasma, and cell culture media samples and analyzed with this kit.

Sample Type	N	Average Linearity	Average Spike Recovery
Serum	4	103	84
Plasma	12	93	96
Cell culture supernatant	1	103	81

**Intra-Assay Precision:** Two samples with different concentrations of mouse CCL11 were tested with 16 replicates in one assay.

	Sample 1	Sample 2
Number of Replicates	16	16
Mean Concentration (pg/mL)	190.5	18.7
Standard Deviation	9.0	1.4
% CV	4.7	7.5

**Inter-Assay Precision:** Two samples with different concentrations of mouse CCL11 were assayed in four independent assays by four operators.

	Sample 1	Sample 2
Number of Assays	4	4
Mean Concentration (pg/mL)	215.2	21.3
Standard Deviation	17.2	3.2
% CV	8.0	15.0

# LEGEND MAX™ Mouse CCL11 ELISA Kit

## Biological Samples:

### *Serum and plasma*

Serum and plasma (Heparin, EDTA, and Citrate) samples of the following strains were pooled from a minimum of ten mice each. All samples were tested for endogenous CCL11. The concentrations measured are shown below:

Strain	Serum	Heparin Plasma	EDTA Plasma	Citrate Plasma
C57BL/6 (pg/mL)	863.5	1565.0	412.5	653.5
BALB/c (pg/mL)	450.5	937.5	848.0	1413.0
Swiss Webster (pg/mL)	337.0	947.0	35.5	472.5
CD-1 (pg/mL)	1150.5	869.0	132.5	535.5

### *Cell culture supernatant*

NIH3T3 cells were established in DMEM/10% FBS culture media at a concentration of  $1 \times 10^6$ /mL, and stimulated with combinations of TNF $\alpha$  (1  $\mu$ g/mL), IL-4 (50  $\mu$ g/mL), and IL-13 (50  $\mu$ g/mL) as indicated. A culture of unstimulated cells was used as a control. Supernatants from each culture were collected on day 3. The concentrations of CCL11 in supernatant measured are shown in the table below.

Sample Type	Treatment	Time	Concentration (ng/mL)
NIH3T3 cell supernatant	Unstimulated	Day 3	0.4
	TNF $\alpha$ +IL-4	Day 3	4.2
	TNF $\alpha$ +IL-13	Day 3	5.5
	TNF $\alpha$ +IL-4 + IL-13	Day 3	4.2

**Troubleshooting Guide:**

<b>Problem</b>	<b>Probable Cause</b>	<b>Solution</b>
High Background	Background wells were contaminated	Avoid cross-well contamination by using the provided plate sealers. Use multichannel pipettes and change tips between pipetting samples and reagents.
	Insufficient washes	Increase number of washes. Increase soaking time between washes prior to addition of substrate solution.
	TMB Substrate Solution was contaminated	TMB Substrate Solution should be clear and colorless prior to addition to wells. Use a clean container prior to pipetting substrate solution into wells.
No or poor signal	Detection Antibody, Avidin-HRP or Substrate solution were NOT added	Rerun the assay and follow the protocol.
	Wrong reagent or reagents were added in wrong sequential order	
	Insufficient plate agitation	The plate should be agitated during all incubation steps using a plate shaker at a speed where solutions in wells are within constant motion without splashing.
	The wash buffer contains Sodium Azide (NaN <sub>3</sub> )	Avoid Sodium Azide contamination in the wash buffer as it inhibits HRP activity.
	Incubations were done at an inappropriate temperature, timing or without agitation	Rerun the assay and follow the protocol.
Low or poor standard curve signal	The standard was incorrectly reconstituted or diluted	Adjust the calculations and follow the protocol.
	Standard was inappropriately stored	Store the reconstituted standard stock solution in polypropylene vials at -70°C. Avoid repeated freeze-thaw cycles.
	Reagents added to wells with incorrect concentrations	Check for pipetting errors and the correct reagent volume.

LEGEND MAX™ Mouse CCL11 ELISA Kit

Problem	Probable Cause	Solution
Signal is high, standard curves have saturated signal	Standard reconstituted with less volume than required	Reconstitute new lyophilized standard with the correct volume of solution recommended in the protocol.
	Standards/samples, detection antibody, Avidin-HRP or substrate solution were incubated for too long	Rerun the assay and follow the protocol.
Sample readings are out of range	Samples contain no or below detectable levels of the analyte	If samples are below detectable levels, it may be possible to use a larger sample volume. Contact technical support for appropriate protocol modifications.
	Samples contain analyte concentrations greater than highest standard point	Samples may require dilution and analysis.
High variation in samples and/or standards	Multichannel pipette errors	Confirm that pipette calibrations are accurate.
	Plate washing was not adequate or uniform	Ensure pipette tips are tightly secured. Ensure uniformity in all wash steps.
	Non-homogenous samples	Thoroughly mix samples before assaying.
	Samples may have high particulate matter	Remove particulate matter by centrifugation.
	Cross-well contamination	Do not reuse plate sealers.  Always change tips for reagent additions. Ensure that pipette tips do not touch the reagents on the plate.

ELISA Plate Template												
	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												



LEGEND MAX™ Kits are manufactured by **BioLegend Inc.**  
9727 Pacific Heights Blvd.  
San Diego, CA 92121  
Tel: 1.858.768.5800  
Tel: US & Canada Toll-Free: 1.877.Bio-Legend (1.877.246.5343)  
Fax: 1.877.455.9587  
Email: [info@biolegend.com](mailto:info@biolegend.com)  
[biolegend.com](http://biolegend.com)

For a complete list of world-wide BioLegend offices and distributors,  
please visit our website at: [biolegend.com](http://biolegend.com)