


## **Purified anti-Keratin 1 Antibody**

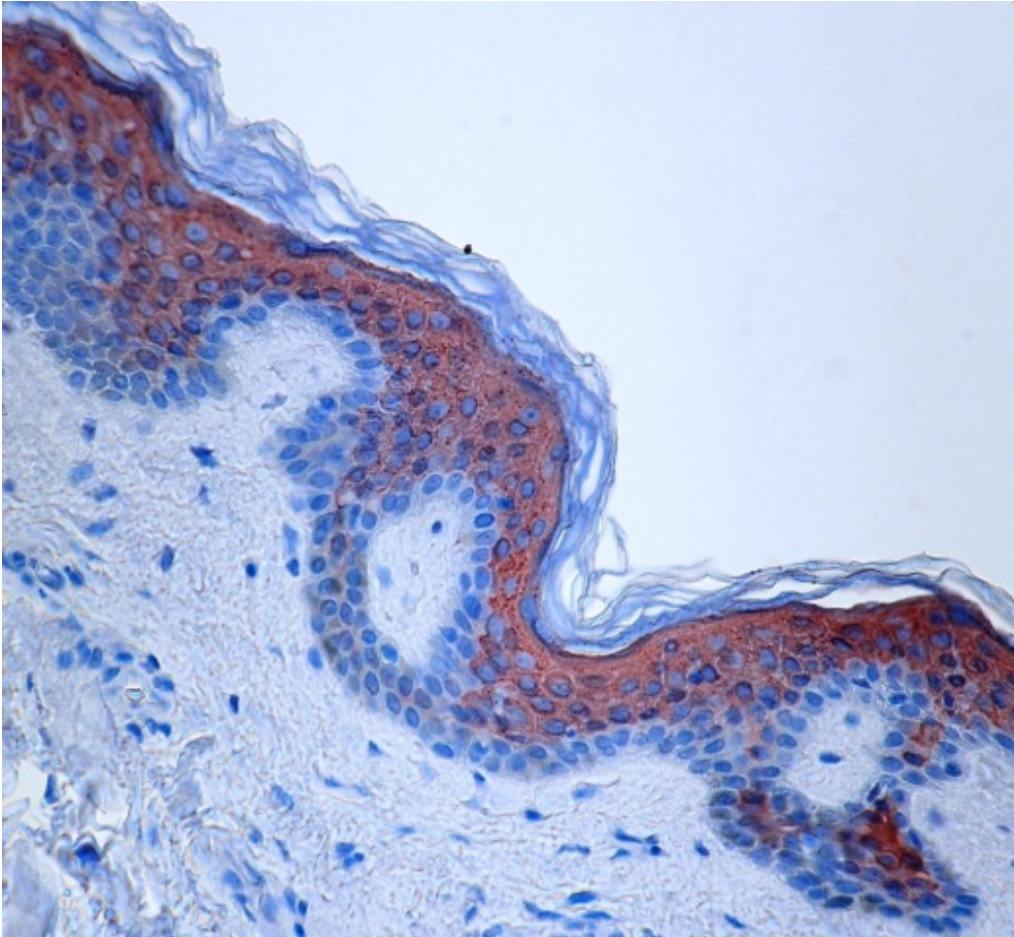

IHC staining of anti-Keratin 1 antibody (Poly19052) on formalin-fixed paraffin-embedded normal human skin. After antigen retrieval using sodium citrate, the tissue was incubated with the primary antibody at 1  $\mu\text{g}/\text{ml}$  for 60 minutes at room temperature. BioLegend's Ultra Streptavidin (USA) HRP Detection Kit was used for detection followed by hematoxylin counterstaining.